

1/16

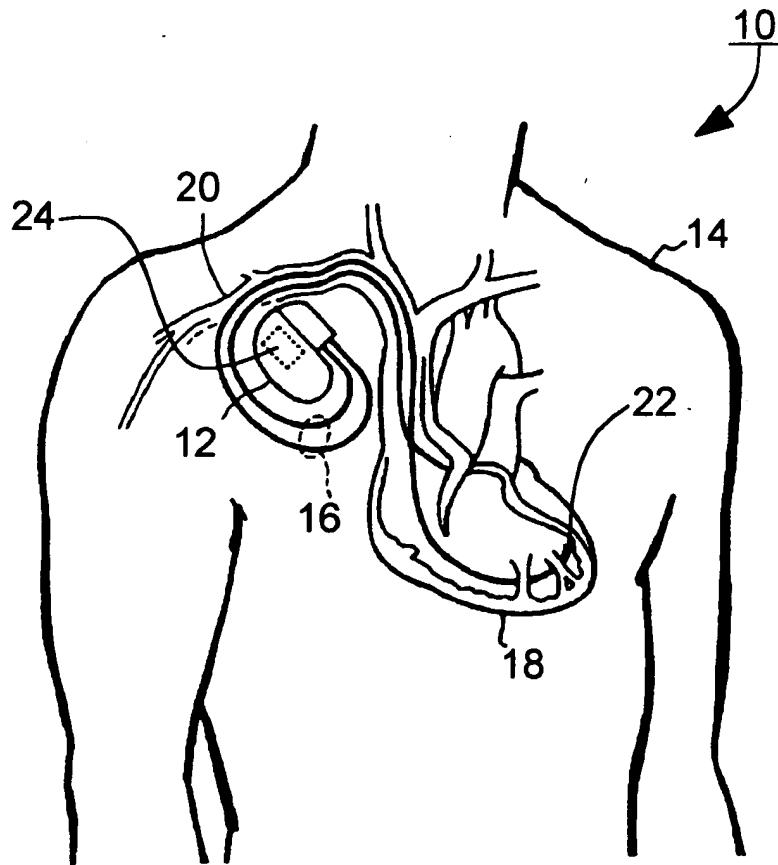


Figure 1

2/16

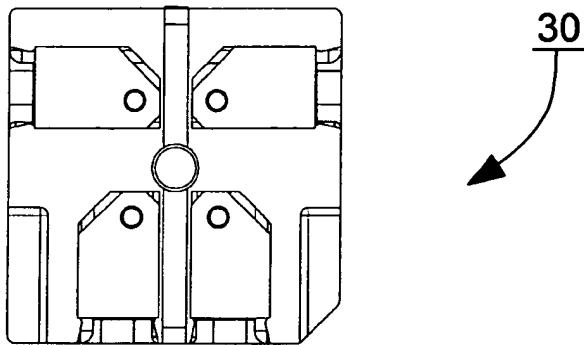


Figure 2A

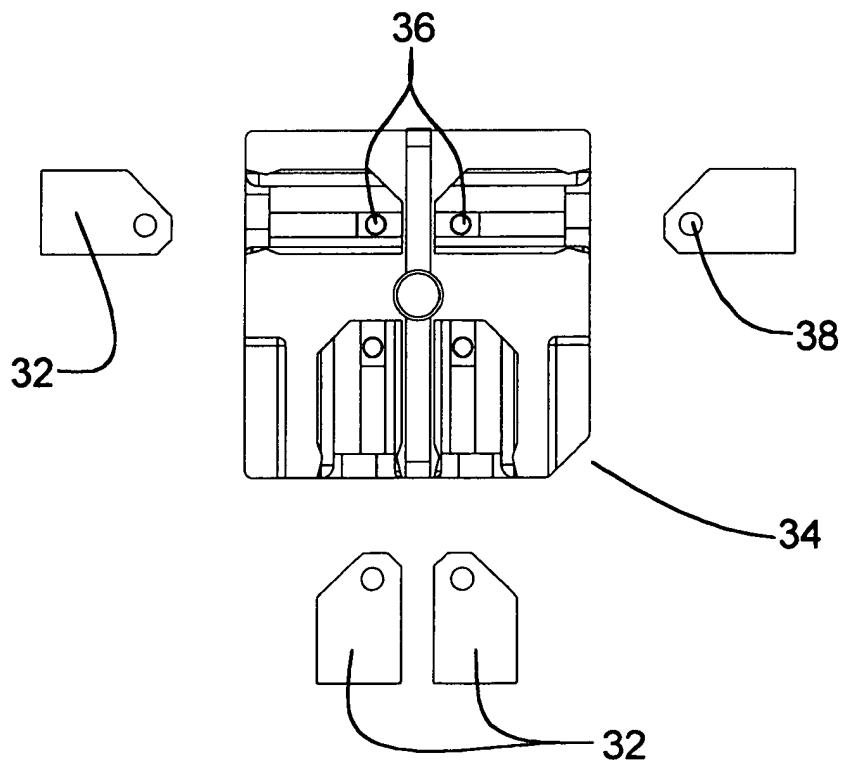


Figure 2B

3/16

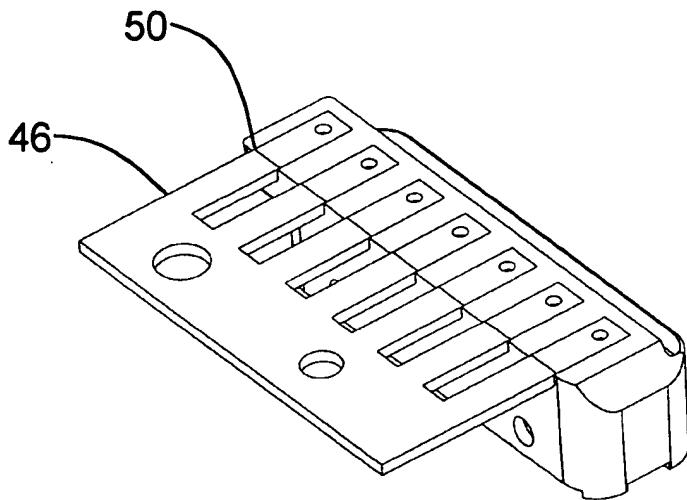


Figure 3A

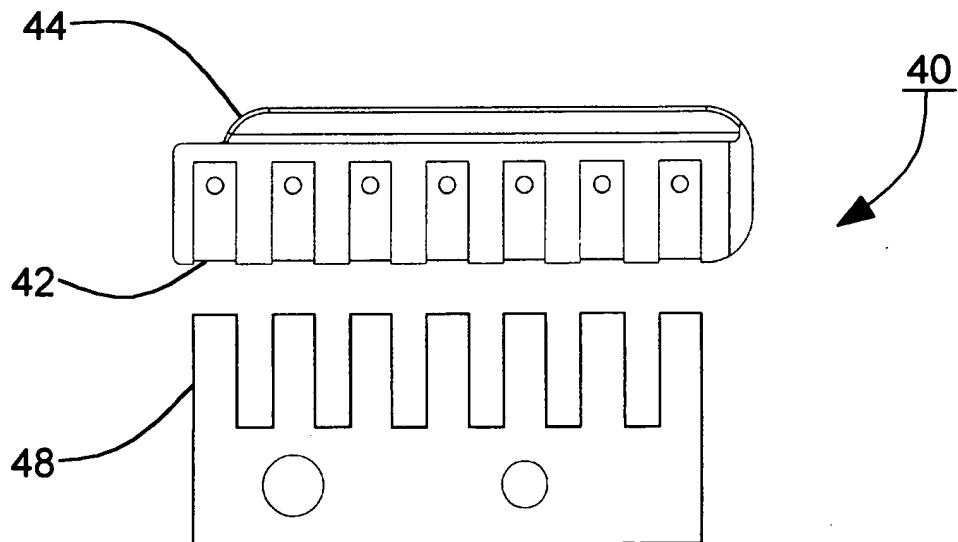


Figure 3B

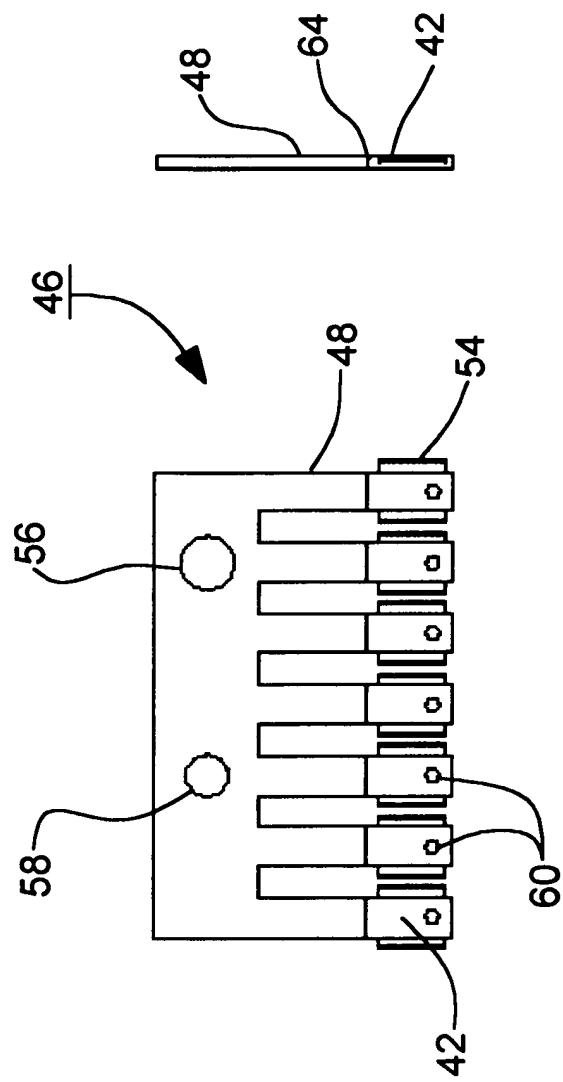


Figure 4B

Figure 4A

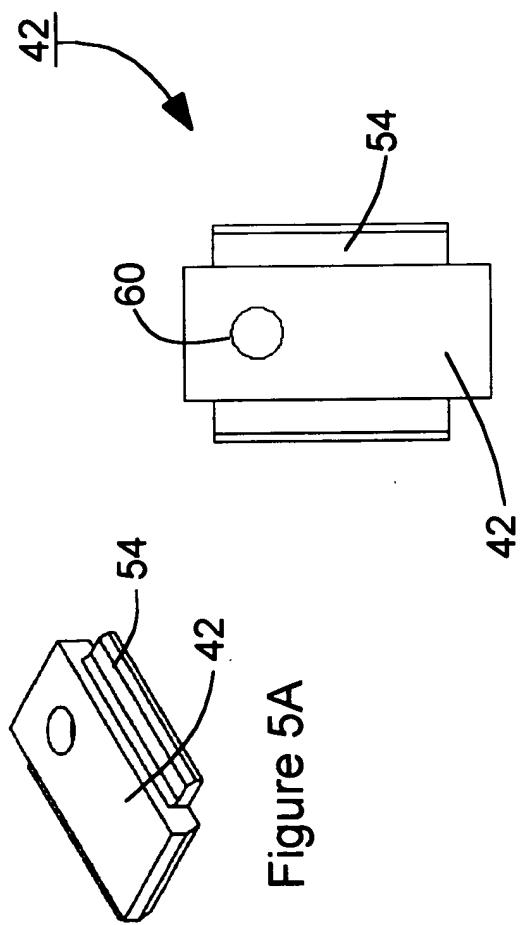


Figure 5A

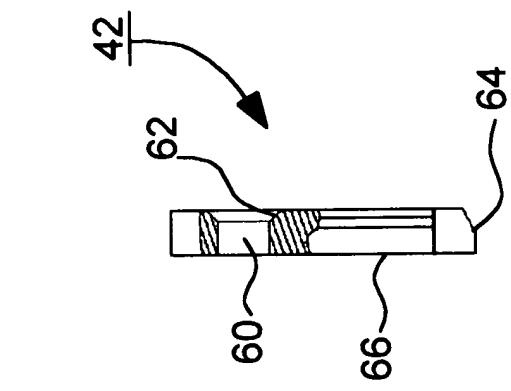


Figure 5B

Figure 5C




Figure 5D

6/16

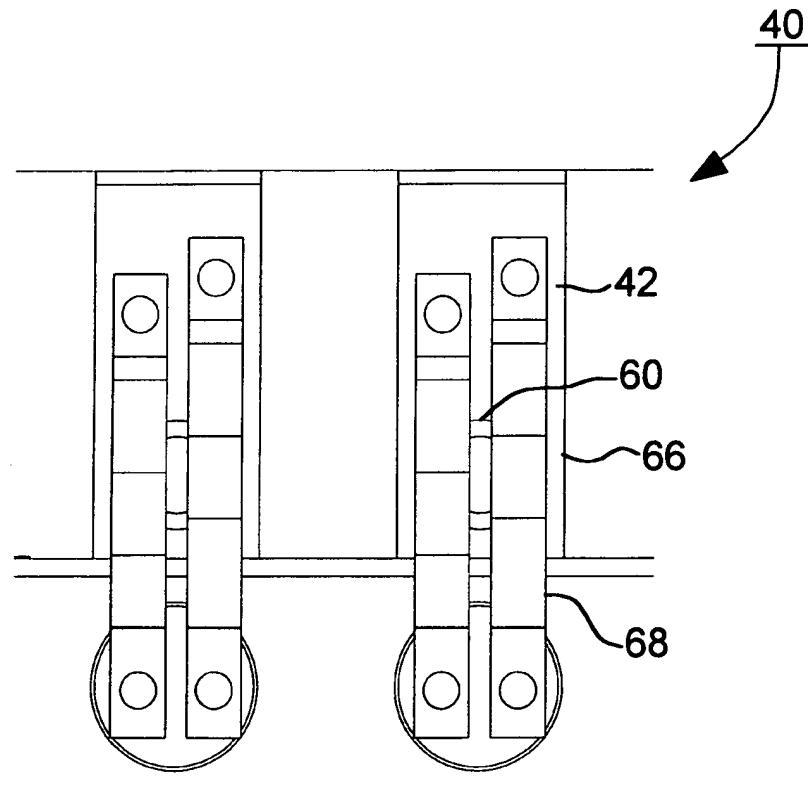


Figure 6

7/16

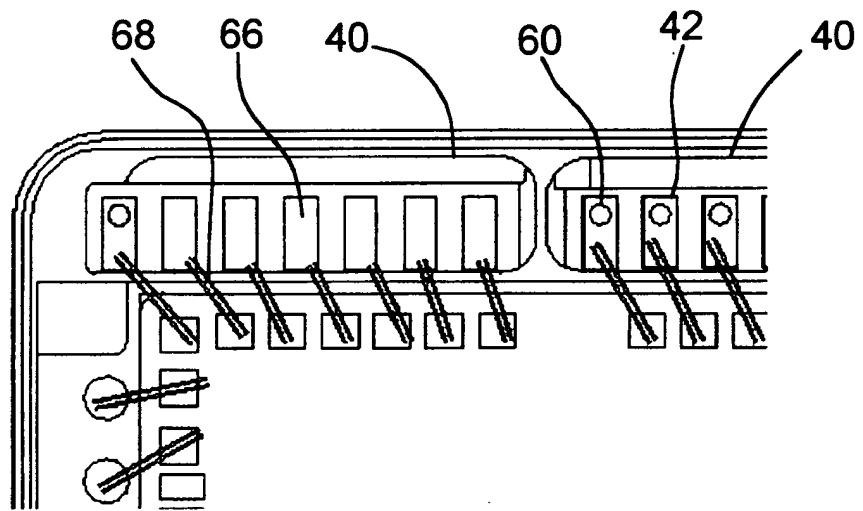


Figure 7

8/16

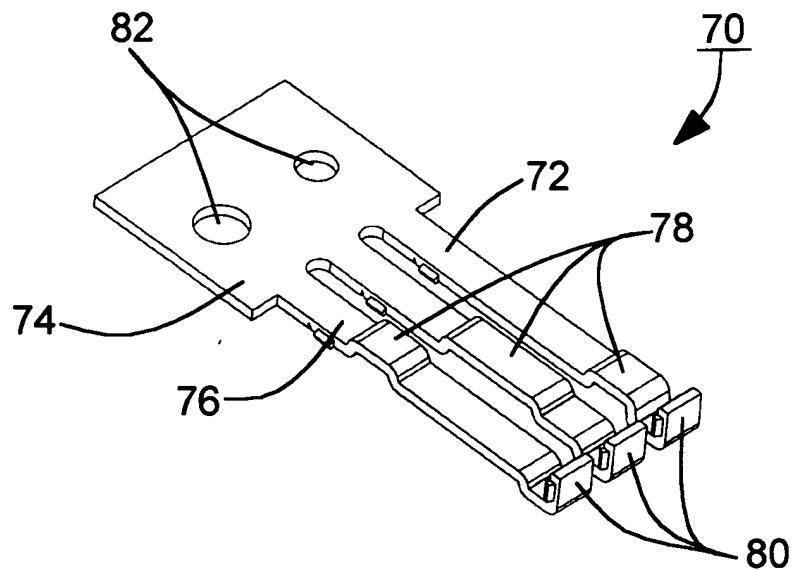


Figure 8A

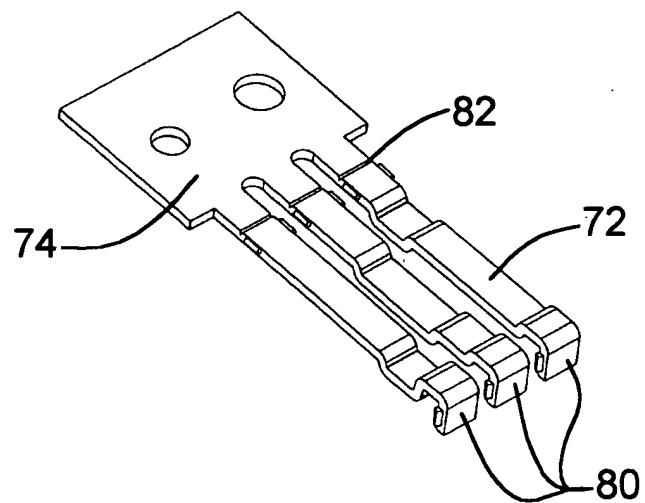


Figure 8B

9/16

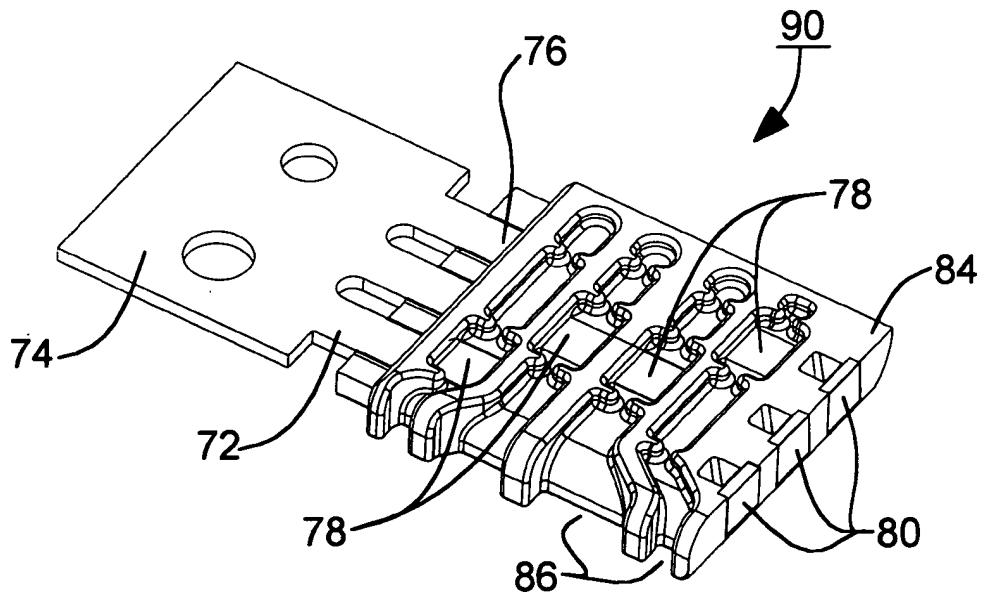


Figure 9A

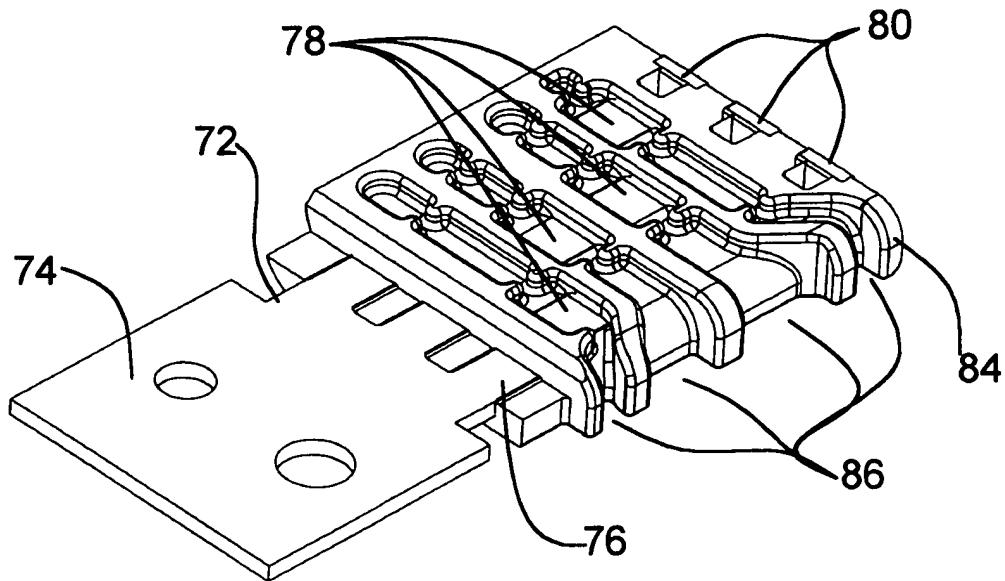


Figure 9B

10/16

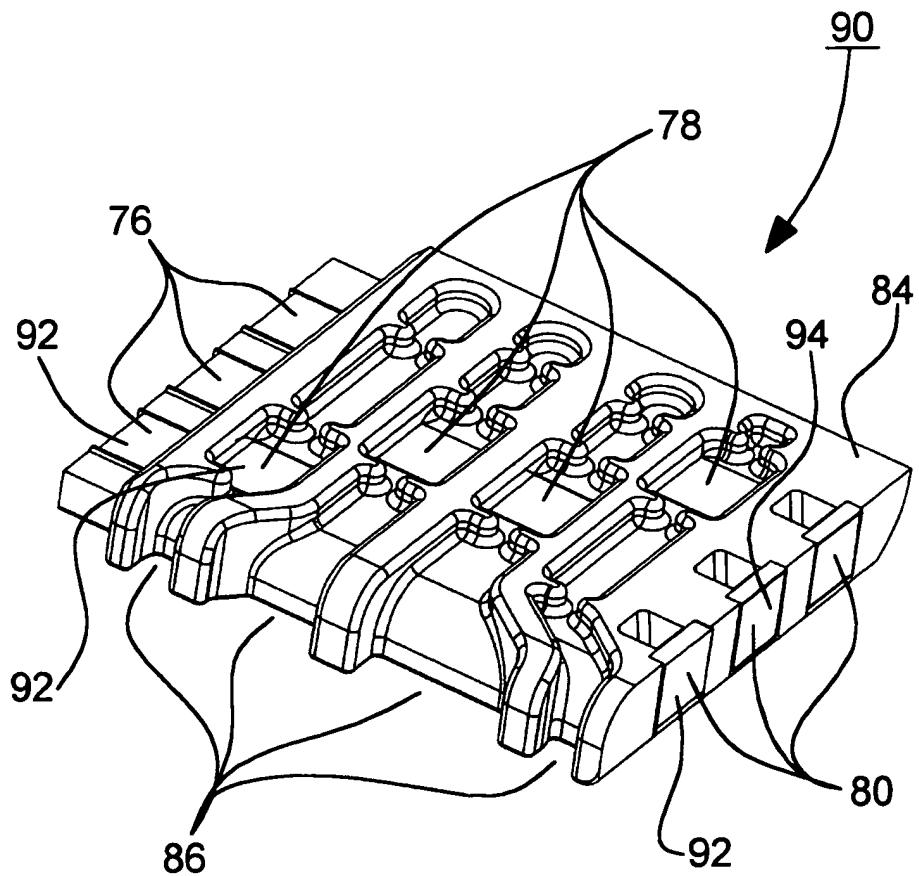


Figure 10

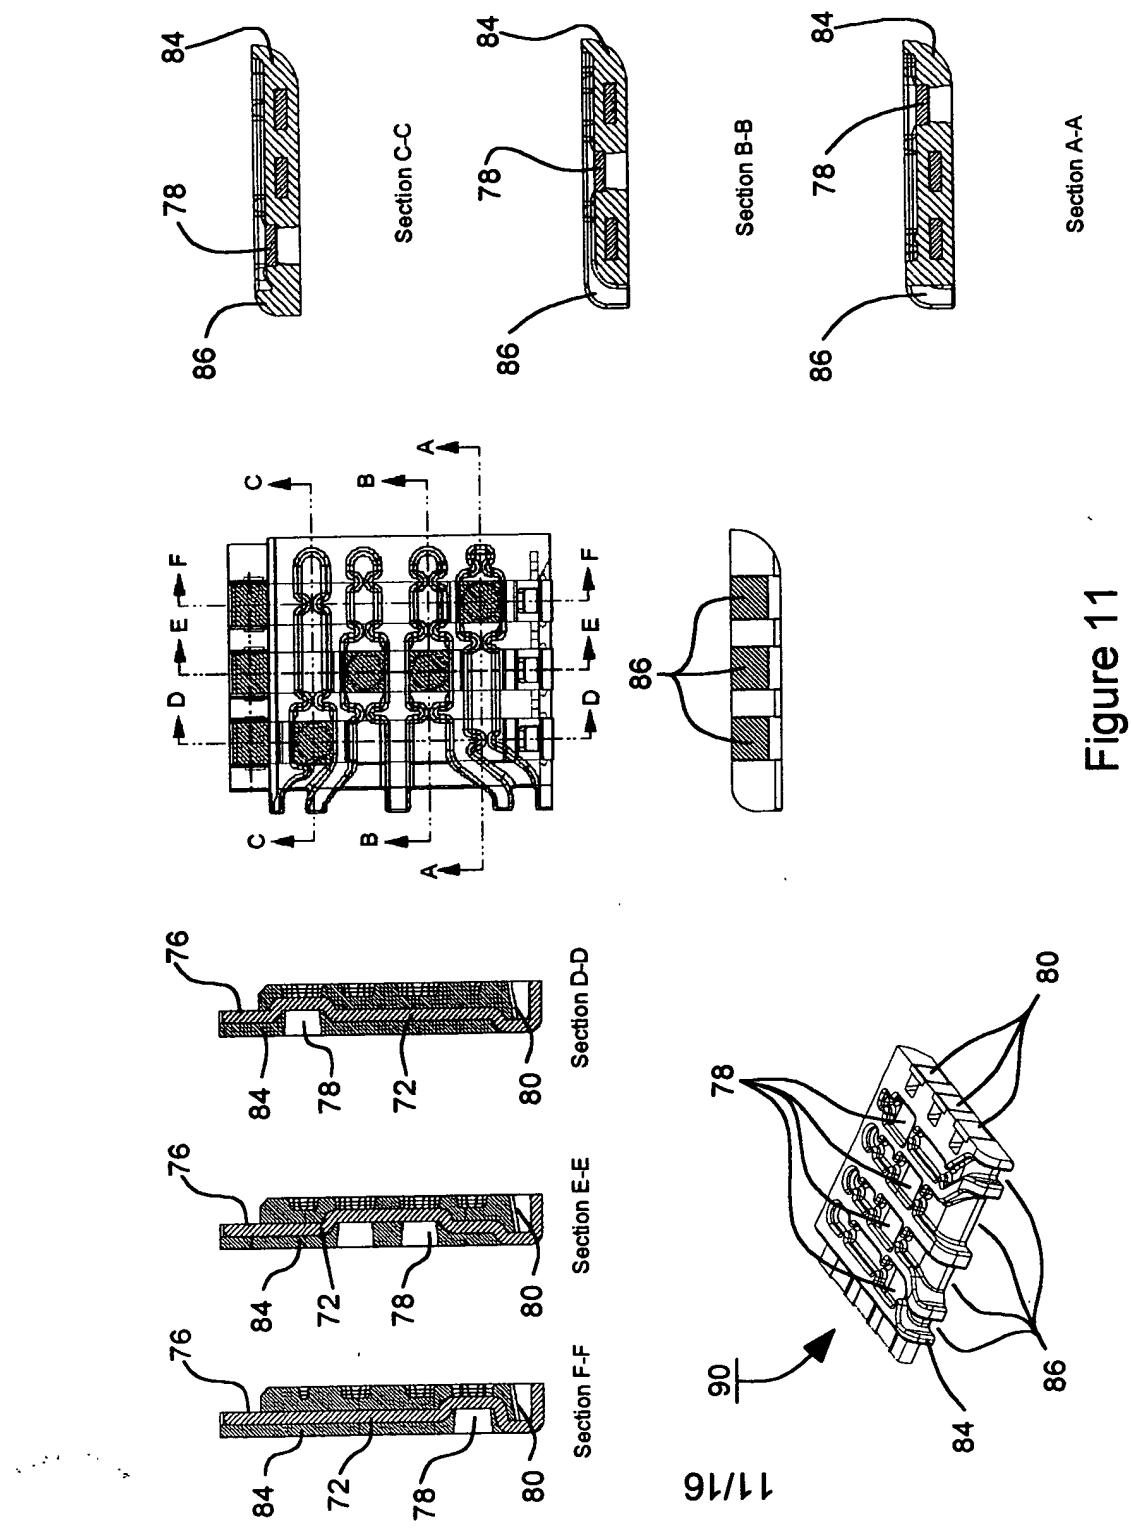


Figure 11

METRONIC, INC. 7MLLE LEAD FRAME AND STRIP MOLDING FOR CONTACT CONNECTORS IN PLATINUM MEDICAL DEVICES
APPLICANT: Robinson et al. SERIAL NO. 10055340
DOCET NO. 442274 SEARCH NO. 11-05-13

12/16

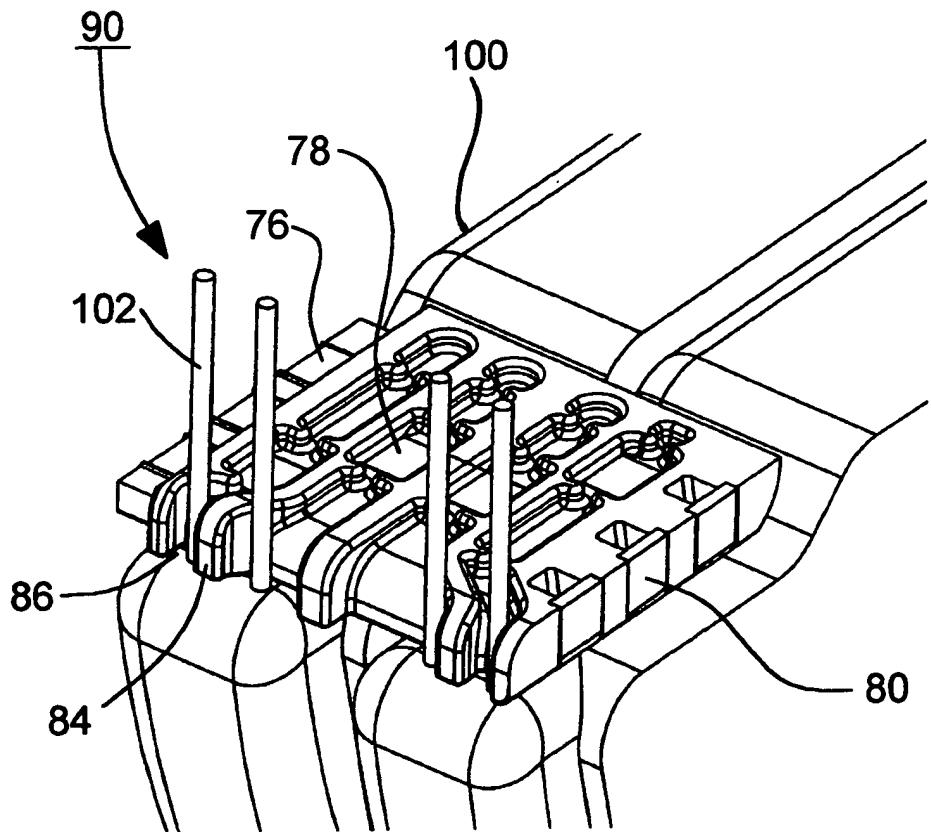


Figure 12

13/16

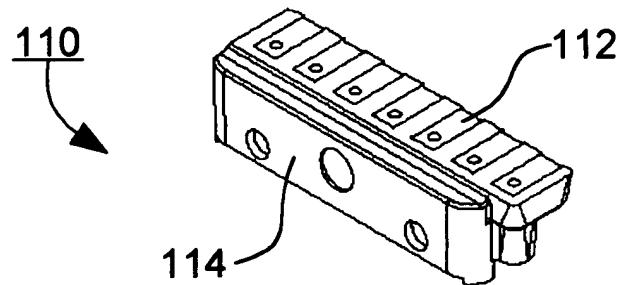


Figure 13A

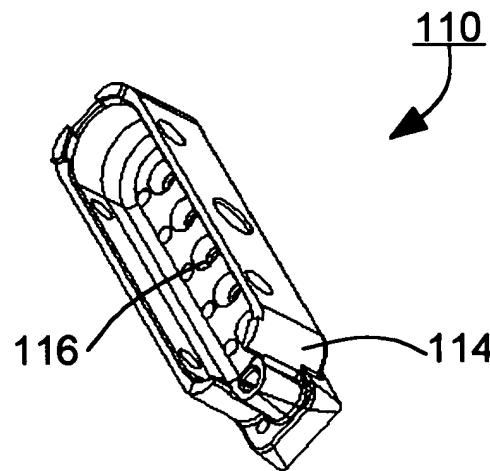


Figure 13B

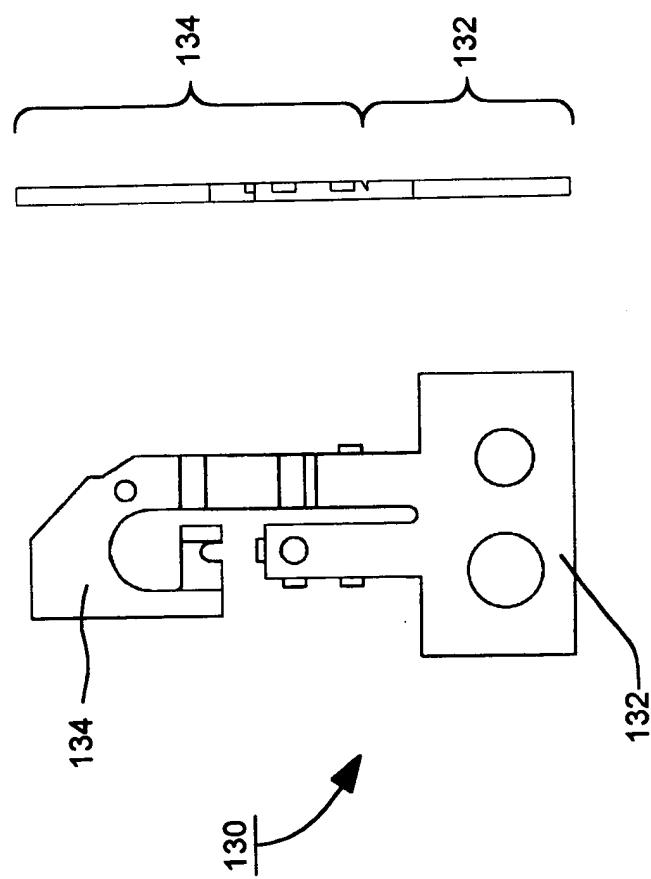


Figure 14

14/16

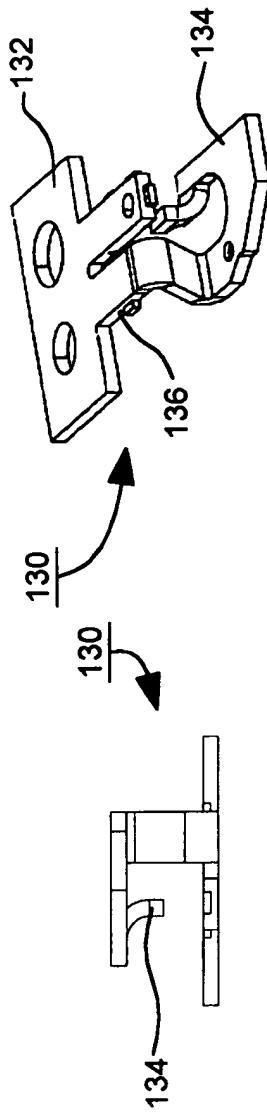


Figure 15A

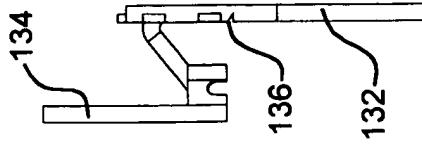


Figure 15B

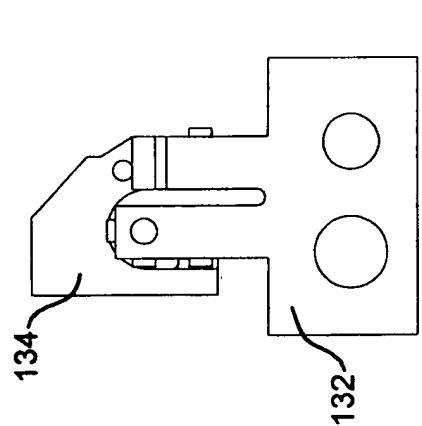


Figure 15C

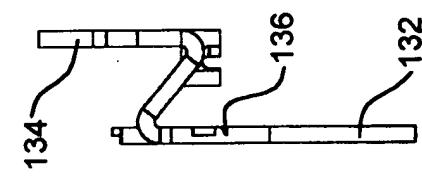


Figure 15D

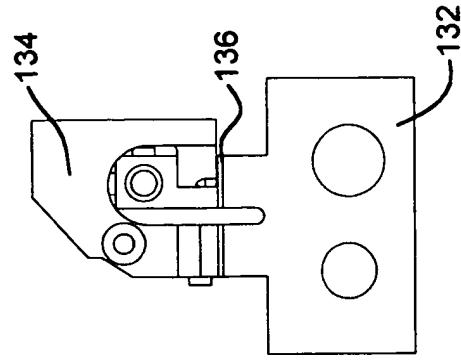


Figure 15E

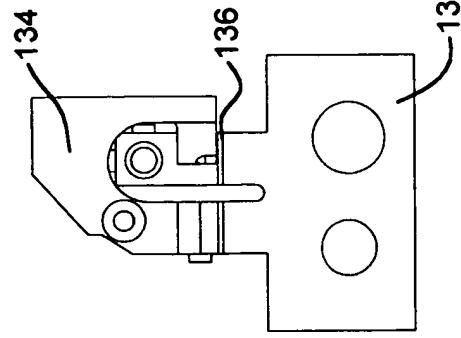


Figure 15F

16/16

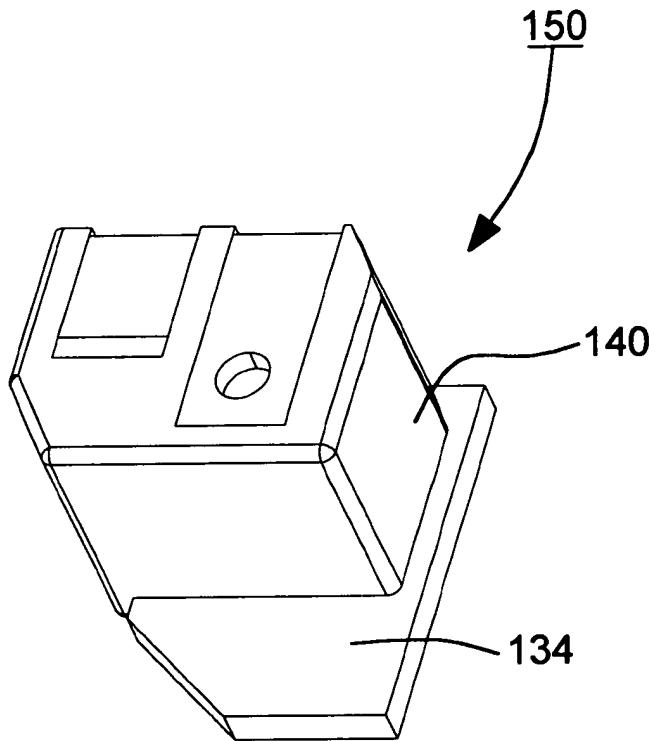


Figure 16